



Kettle Tester Model 6280

Friborg Test Technology AB

Mail address

P.O. Box 63
SE-196 22 Kungsängen
Sweden

Visiting address


Kraftvägen 32
SE-196 37 Kungsängen
Sweden

T: +46 (0) 8 581 610 10
F: +46 (0) 8 505 961 50

info@friborg.se
www.friborg.se

Technical Specification

- Consist of PLC, on/off buttons for cylinder movement, specimen placement, pumps and water tank of 20 litre
- PLC controls the pneumatic cylinders, pumps, water temperature, time and counts cycles/periods
- The Kettle is operated empty at 0,85 or 1,15 times rated power input
- Within 2 sec of the other thermal cut-out operating, the Kettle is filled with water having a temperature of $15\text{ °C} \pm 5\text{ °C}$
- After one (1) minute, the Kettle is emptied
- The test is carried out 100 times

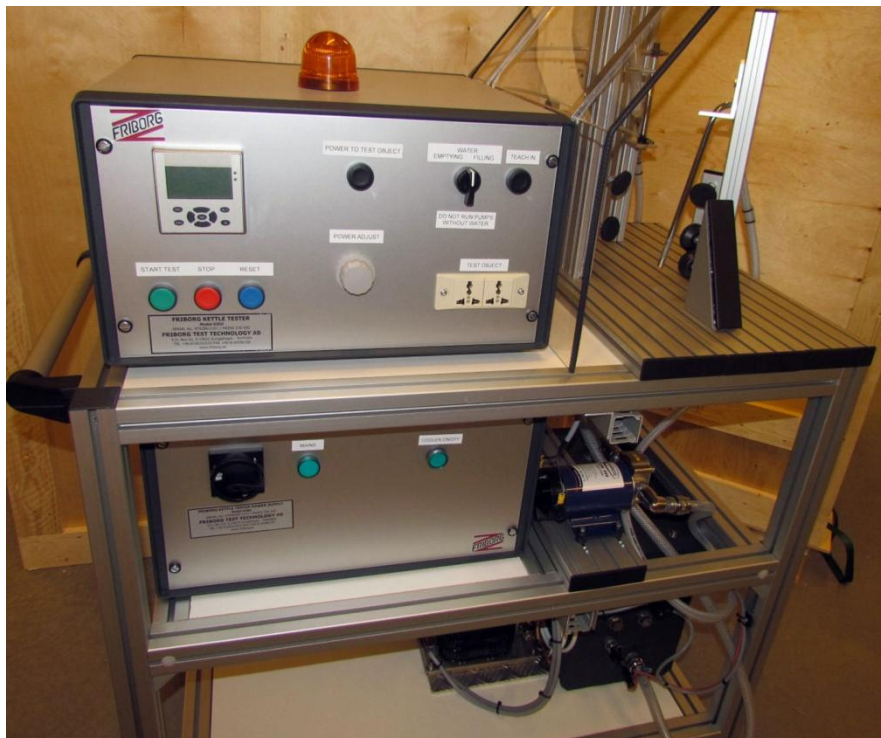

Facts

Standard:

IEC 60335-2-15 Clause 19.102

Components:

-

Weight:

App. 150 kg

Dimensions:

1200x800x1400 mm (LxWxH)

Supply

230 VAC, 50/60 Hz, 10 A

Air supply 6 bar